


Andover Corporation

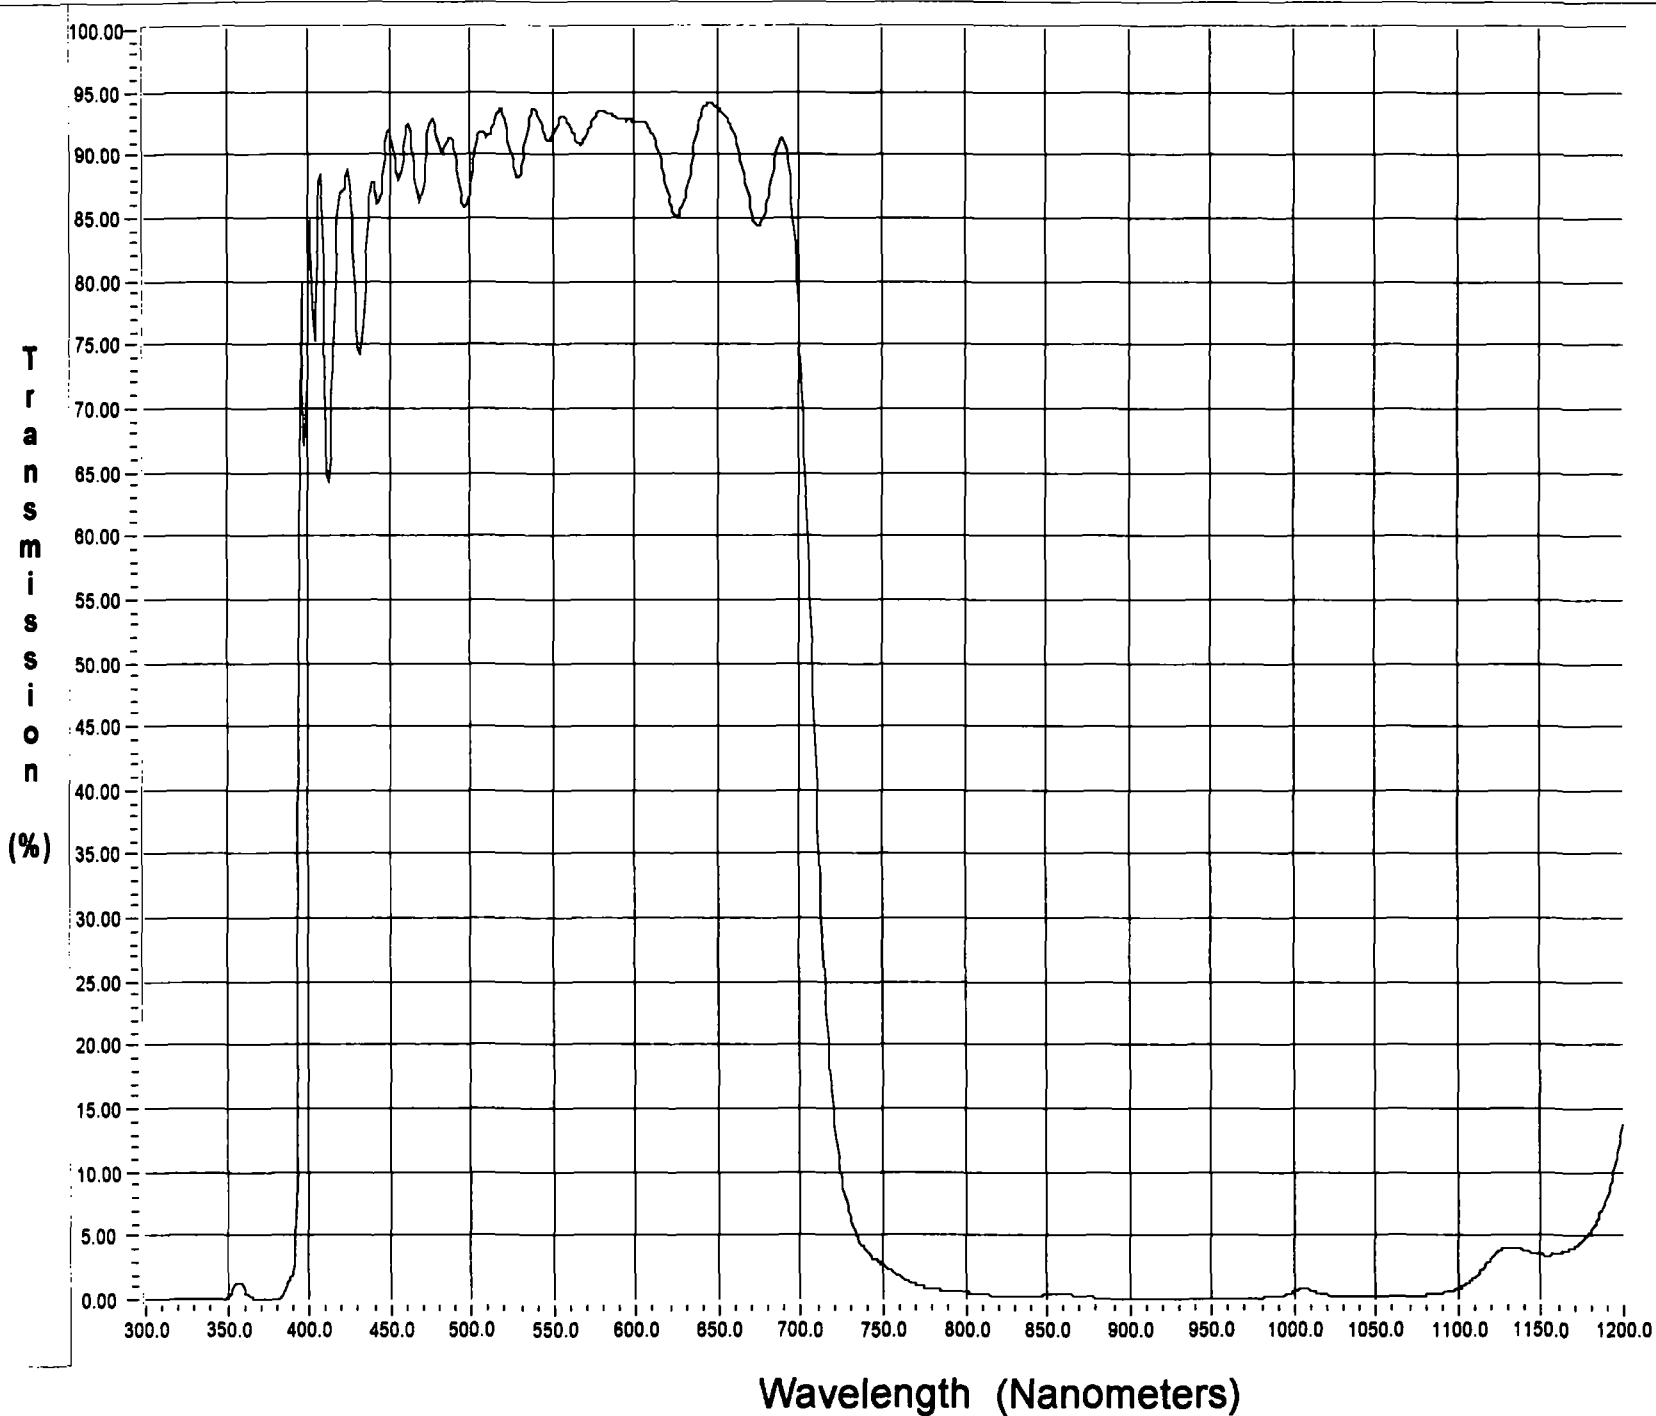

Filter I.D.

Test Instrument:

Cary 500 (1437)

Test Technician:

J. Moreau *jcm*

Date:

Fri, Aug 29, 2003

Customer Name:

University of California

Job Number:

AM-53808

Part Number:

ANDV8970

Serial Number:

01

Lot Number:

21161

Filter Data

Transmission average from:

450nm - 675nm: 90.852%

750nm - 1200nm: 1.234%

Polarization:

RANDOM

Angle of Incidence:

0.00°

Ambient Temperature:

23.0 ° C.



Andover Corporation

4 Commercial Drive, Salem, NH 03079 USA
Telephone: (603) 893-6888 Fax: (603) 893-6508

Web site: www.andcorp.com
e-mail: crichards@andcorp.com

Christopher A. Richards
Quality Control Manager

Optical components for research and industry